



Zimmer Biomet Sports Medicine designed, developed, and launched the first all-suture anchor on the market, known as the JuggerKnot® Soft Anchor. Once surgeons began utilizing this anchor they quickly realized how useful the implant is for hip labral repairs. Therefore, while working alongside these surgeons, a complete set of hip arthroscopy instrumentation has been developed to complement the innovative anchor technology.

The Zimmer Biomet Sports Medicine hip arthroscopy instrumentation is designed specifically for arthroscopic hip procedures. The size and shape of each individual instrument was carefully designed with the hip anatomy in mind and crafted from durable stainless steel material.



Access the Joint



Portal Management Instrumentation

HydroDam™ Cannula System

- Dual Seal Design: Facilitates smooth implant or instrument passage with minimal leakage
- Translucent body allows for easy visualization of instrumentation and suture
- Turn-key design for out-flow of fluid
- Multiple sizes and lengths for hip and shoulder
- Latex free
- Obturator system is reusable, modular, and cannulated








JuggerKnot Soft Anchor **Implants & Instrumentation**

Centering Sleeve Instrumentation



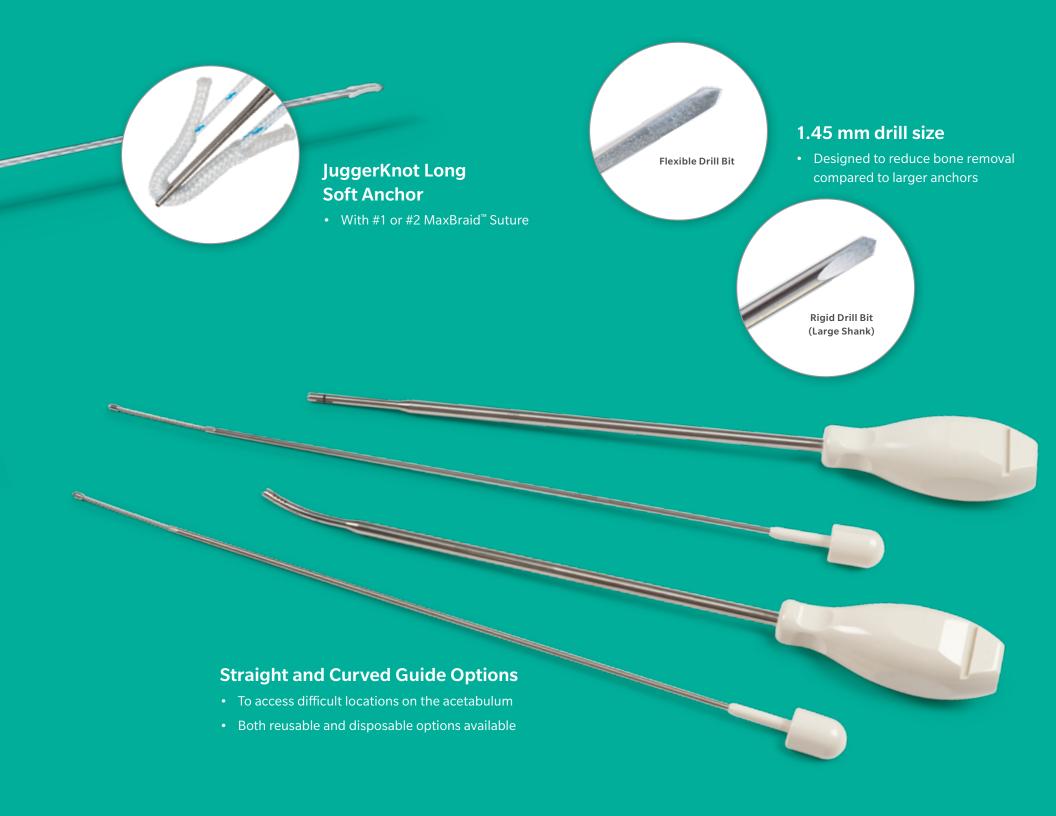




SureLock 1.4mm All-Suture Anchor

- Inserter-Controlled Deployment Method
 - Provides consistent anchor delivery beneath the cortex

Quattro[®] GL Suture Anchor

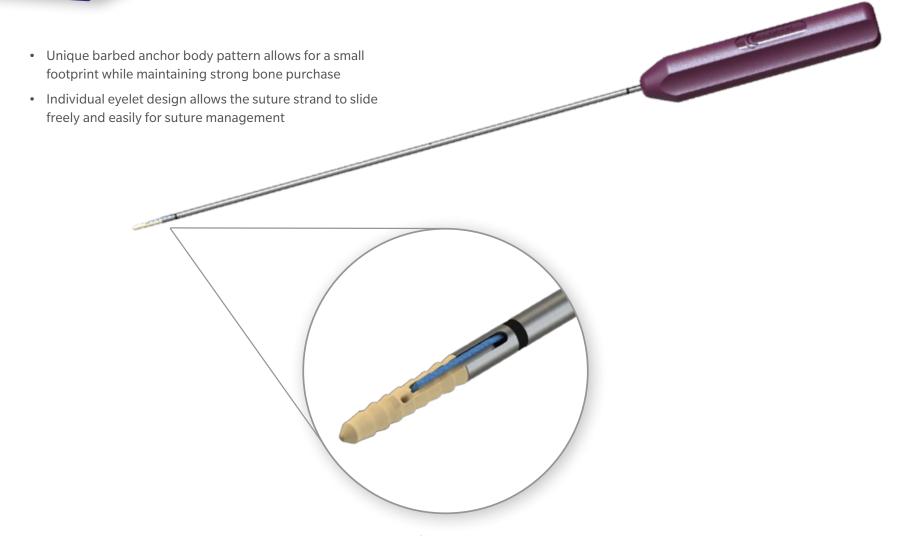

Quattro GL 2.9mm Suture Anchor

• PEEK-OPTIMA® Push-in Anchor is single-loaded with #2 Suture



Suture Retrieval Suture Sliding

Suture Locking

Hip Arthroscopy

Dragon Tongue Suture Passing Device for Capsular Closure

Extended Delivery

- Adjustable slide delivers 30 mm of suture, creating an easily graspable suture loop.
- Designed for single portal capsular repair and is not dependent on angle of approach.

Range of Reach

- Easily capture the delivered suture loop in near and far positions with both grasping capabilities.
- Nitinol grasper can open and close along its 17 mm of extension beyond the needle shaft.





Variable Angles

• Nitinol grasper advances out of the needle shaft at 60° and continues to extend further to a 70° bend.





Zimmer Biomet Sports Medicine Hip Arthroscopy Instrumentation


The beauty of this instrumentation is the ability to mix and match certain instruments required for specific procedures. The bottom four caddies have the ability to be swapped out depending upon surgeon preference.

Hip instrument caddy options include:

- Hand Instruments
- JuggerKnot Long
- Microfracture

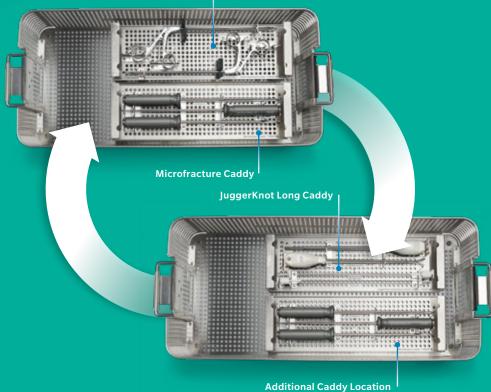

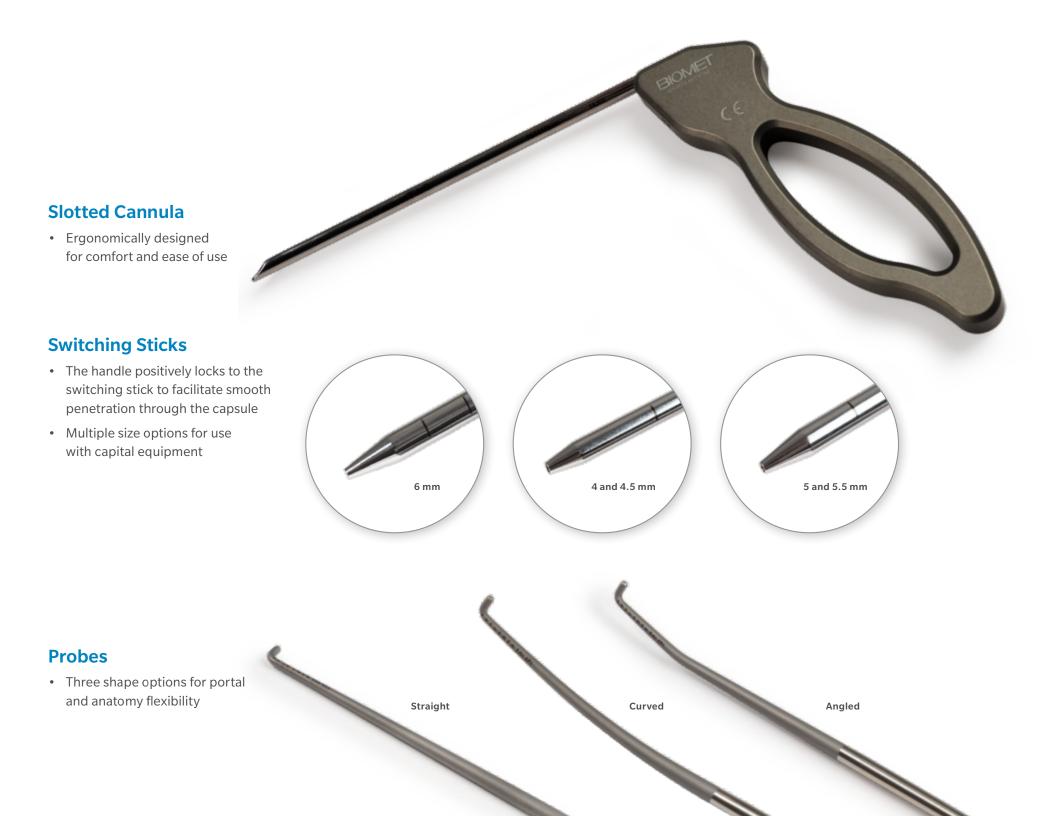

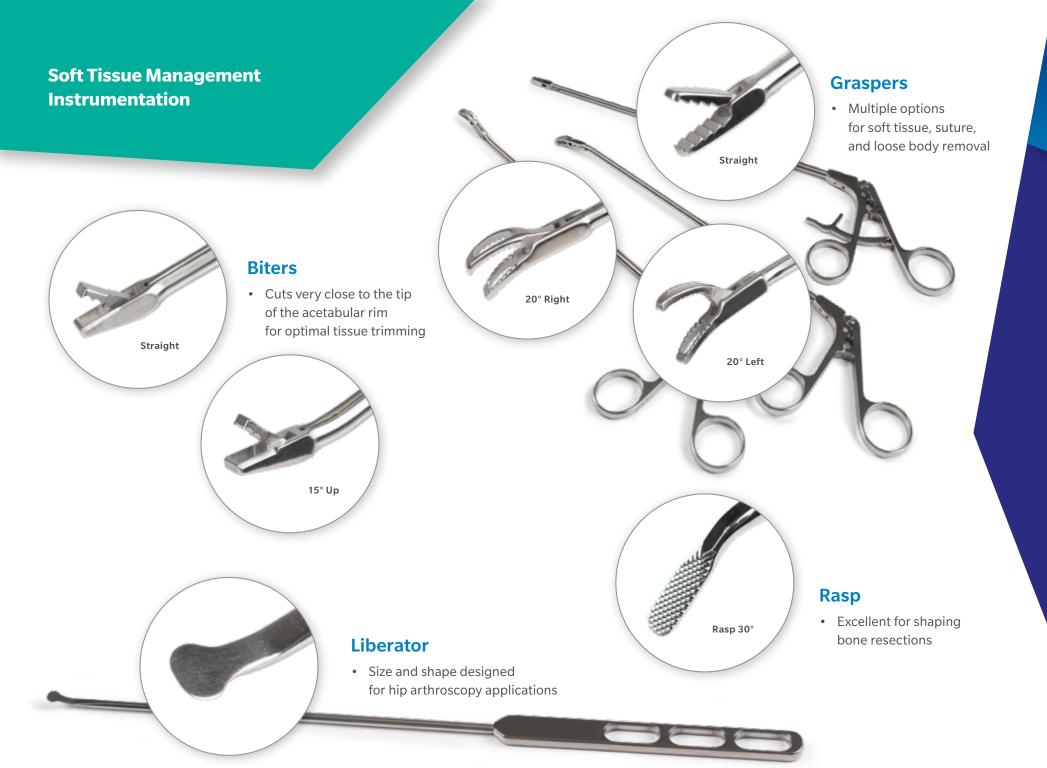

Suture Management Instrumentation





Stitchers/Passers

- Low profile design with multiple tip geometries
- Right and left Stitcher options available
- Straight and 35° Up Passer options available


Knot Pusher

• Length designed for hip arthroscopy



Manipulator/Grasper


• Hold and manipulate sutures



Cutter

• Easily disassembled for efficient cleaning



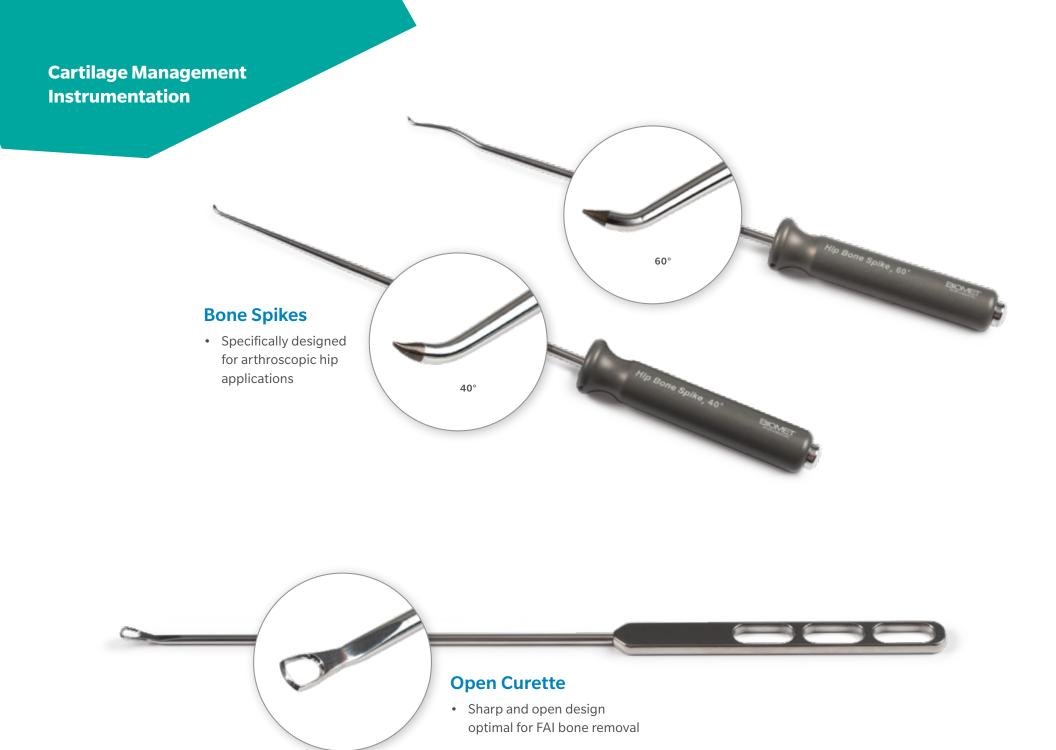

Ordering Information

Access the Joint

Part Number	Description
640410BSM	Hip Access Kit (2 Access Needles & 2 Nitinol Guide Wires)
640420BSM	Hip Access Kit with Curved Blade, Blunt Tip
640430BSM	Hip Access Kit with Straight One Sided Blade, Blunt Tip
640431BSM	Hip Access Kit with Curved Blade, Sharp Tip
641410BSM	Hip Access System (2 Access Needles, 2 Nitinol Guide Wires, 30 CC Syringe, & Marking Pen & Ruler)
641420BSM	Hip Access System with Curved Blade, Blunt Tip
641430BSM	Hip Access System with Straight One Sided Blade, Blunt Tip
641431BSM	Hip Access System with Curved Blade, Sharp Tip
169420BSM	Curved Blade, Blunt Tip
169430BSM	Straight One Sided Blade, Blunt Tip
169431BSM	Curved Blade, Sharp Tip

Portal Management Instrumentation

Part Number	Description
754440FBSM	Hip 4.5 mm Cannulated Switching Stick
754450FBSM	Hip 5.0 mm Cannulated Switching Stick
754410BSM	Hip 6 mm Slotted Cannula
754420FBSM	Hip 4 mm Cannulated Switching Stick
754430FBSM	Hip Switching Stick Handle
754470FBSM	Hip 6 mm Cannulated Switching Stick
754480FBSM	Hip 5.5 mm Cannulated Switching Stick
138405BSM	Hip Straight Probe
138415BSM	Hip Curved Probe
138416BSM	Hip Angled Probe
110019086	HydroDam Rigid Cannula 8.5 x 115 mm Single pk
110019090	HydroDam Rigid Cannula 8.5 x 100 mm Single pk
110030950	HydroDam Rigid Cannula 8.5 x 130 mm Single pk

Ordering Information (cont.)

JuggerKnot Long Soft Anchor Implants

Part Number	Description
916030	JuggerKnot Long Soft Anchor #1 Single Loaded
010000334	JuggerKnot Long Soft Anchor #1 10pk
010000324	JuggerKnot Long Soft Anchor #2 Single Loaded
010000335	JuggerKnot Long Soft Anchor #2 10pk

JuggerKnot Long Soft Anchor Instrumentation

Part Number	Description
110002759	Reusable Straight Fishmouth Guide
916020	Curved Disposable Set (Guide, Centering Sleeve, and Flexible Drill Bit)
916034	Reusable Curved Guide
916035	Reusable Straight Four-Prong Guide
916036	Disposable Flex Drill
916037	Disposable Rigid Drill
916038	Reusable Trocar
916039	Reusable Obturator
916040	Disposable Straight Set (Guide and Rigid Drill)
110016992	Disposable Flex Drill with Centering Sleeve

SureLock All-Suture Anchor

Part Number	Description	
CM9614F	SureLock 1.4mm Flex Anchor	
SureLock All-S	uture Disposables	
Part Number	Description	
CM9640	SureLock 1.4mm Drill	

SureLock 1.4mm AS Drill w/ Centering Sleeve

SureLock All-Suture Instruments

CM9640S

Part Number	Description
CM9641	SureLock 1.4mm Obturator
CM9643	SureLock 1.4mm Straight Drill Guide
CM9645	SureLock 1.4mm Curved 25D Drill Guide

Quattro GL 2.9mm Suture Anchors

Part Number	Description
CM9329	Quattro 2.9mm GL Anchor

Quattro GL Disposables

Part Number	Description
CM9300ST	Quattro Spade Drill
CM9324ST	Quattro Fluted Hard Bone Drill

Quattro GL Instruments

Part Number	Description
CM9301	Quattro 2.9mm Drill Guide
CM9302	Quattro 2.9mm Obturator Blunt

Ordering Information (cont.)

Suture Management Instrumentation

Part Number	Description
110030129	SpeedSnare Suture Passer 30° Up
110030130	SpeedSnare Suture Passer 60° Up
110030131	SpeedSnare Suture Passer 30° Right
110030132	SpeedSnare Suture Passer 30° Left
110030133	SpeedSnare Suture Passer Straight
110030140	SpeedSnare Suture Passer 30° Up Reverse
110030141	SpeedSnare Suture Passer 60° Up Reverse
110038984	Dragon Tongue Suture Passer
328412BSM	Hip Stitcher — Right
328422BSM	Hip Stitcher —Left
399400BSM	Hip Suture Passer — Straight
399431BSM	Hip Suture Passer — 35° Up
301400BSM	Hip Knot Pusher
231400BSM	Hip Suture Cutter
601400BSM	Hip Suture Manipulator
602400BSM	Hip Suture Grasper

Soft Tissue Management Instrumentation

Part Number	Description
727400BSM	Hip 3 mm Biter — Straight
727431BSM	Hip 3 mm Biter 15° Up
904131BSM	Hip 20° Tissue Liberator
904431BSM	Hip Rasp 30° Up
391400BSM	Hip 5 mm Grasper — Straight
391411BSM	Hip Grasper 20°— Right
391421BSM	Hip Grasper 20°— Left
397400BSM	Hip Tissue Grasper

Cartilage Management Instrumentation

Part Number	Description	
904441BSM	Hip Curette Bent 20°	
512404BSM	Hip Bone Spike — 60°	
512406BSM	Hip Bone Spike — 40°	

Case and Caddies

Part Number	Description
110024748	Hip Instrument Case
110024749	Hip Instrument Lid
110024750	Hip Instrument Caddy JuggerKnot Long
110024751	Hip Instrument Caddy Hand Instruments
110024752	Hip Instrument Caddy Microfracture

Hip Arthroscopy Instruments:

INTENDED USE

The Hip Arthroscopy Instruments (hereafter hip instruments) are intended to be used in operative arthroscopic procedures in the hip joint.

The hip instruments are reusable instruments.

CONTRAINDICATIONS

The hip instruments are NOT intended for use where one or more of the following conditions exist:

- Pathological conditions of the tissue to be treated.
- Physical conditions that would retard healing, such as blood supply limitation and infection.
- Conditions which tend to limit the patient's ability or willingness to follow instructions during the healing period.

JuggerKnot Soft Anchors:

INDICATIONS FOR USE

The JuggerKnot Soft Anchors are intended for soft tissue to bone fixation for the following indications:

Shoulder

Bankart lesion repair

SLAP lesion repair

Acromio-clavicular repair

Capsular shift/capsulolabral reconstruction

Deltoid repair

Rotator cuff tear repair

Biceps tenodesis

Pectoralis major repair

Foot and Ankle

Medial/lateral repair and reconstruction

Mid and forefoot repair

Hallux valgus reconstruction

Metatarsal ligament/tendon repair or

reconstruction

Achilles tendon repair

Elbow

Ulnar radial collateral ligament reconstruction Lateral epicondylitis repair Biceps tendon reattachment

Knee

Extra-capsular repair:

MCL, LCL, and posterior oblique ligament

Iliotibial band tenodesis

Patellar tendon repair

VMO advancement

Joint capsule closure

MPFL repair or reconstruction

Quadriceps tendon repair

Hip

Acetabular labral repair Proximal hamstring repair

CONTRAINDICATIONS

- 1. Infection.
- 2. Patient conditions including blood supply limitations and insufficient quantity or quality of bone or soft tissue.
- 3. Patients with mental or neurologic conditions who are unwilling or incapable of following postoperative care instructions or patients who are otherwise unwilling or incapable of doing so.
- 4. Foreign body sensitivity. Where material sensitivity is suspected, testing is to be completed prior to implantation of the device.

SureLock® 1.4mm All-Suture

INDICATIONS FOR USE

Anchor Intended Use in the United States

The SureLock All-Suture Anchors are intended to be used for the reattachment of soft tissue to bone for acetabular labral repair.

CONTRAINDICATIONS

- 1. Surgical procedures other than those listed in the INDICATIONS section.
- 2. Presence of infection.
- 3. Patient conditions including insufficient quantity or quality of bone or soft tissue.
- 4. Insufficient blood supply or previous infection which may hinder the healing process.
- 5. Foreign body sensitivity. If material sensitivity is suspected, testing should be completed prior to device implantation.
- The use of this device may not be suitable for patients with immature bone. The physician should carefully assess the device within cartilage epiphyseal growth plates or nonosseous tissue.
- 7. Conditions which may limit the patient's ability or willingness to follow postoperative care instructions.

Quattro® GL 2.9mm Suture Anchor

INDICATIONS FOR USE

The Quattro GL Suture Anchors are intended to be used for the reattachment of soft tissue to bone for capsular repair and acetabular labrum reattachment

CONTRAINDICATIONS

- 1. Surgical procedures other than those listed in the INDICATIONS section.
- 2. Presence of infection.
- 3. Patient conditions including insufficient or immature bone.
- 4. Insufficient blood supply or previous infections which may hinder the healing process.
- 5. Foreign body sensitivity. If material sensitivity is suspected, testing should be completed prior to device implantation.
- 6. The physician should carefully assess the device within immature bone.
- 7. The placement of this device should not impact or disrupt the growth plate.
- 8. Conditions which may limit the patient's ability or willingness to follow postoperative care instructions.

This material is intended for healthcare professionals and the Zimmer Biomet sales force. Distribution to any other recipient is prohibited. For indications, contraindications, warnings, precautions, potential adverse effects and patient counseling information, see the package insert or contact your local representative; visit http://www.zimmerbiomet.com for additional product information. All content herein is protected by copyright, trademarks and other intellectual property rights, as applicable, owned by or licensed to Zimmer Biomet or its affiliates unless otherwise indicated, and must not be redistributed, duplicated or disclosed, in whole or in part, without the express written consent of Zimmer Biomet.

Check for country product clearances and reference product-specific instructions for use.

Not for distribution in France.

T.A.G. Medical Products is the manufacturer of the hip arthroscopic instrumentation, hip access kit, and SpeedSnare. Zimmer Biomet Sports Medicine is the distributor only.

 $Zimmer\ Biomet\ Sports\ Medicine\ is\ the\ manufacturer\ of\ the\ Hip\ Instrument\ Case,\ Hydro\ Dam\ Cannulas,\ and\ Jugger\ Knot\ Soft\ Anchor\ and\ instrumentation.$

©2019, 2021 Zimmer Biomet



Legal Manufacturer

T.A.G. Medical Products, Ltd., Kibbutz Gaaton 2513000 Israel.



Legal Manufacturer

Cayenne Medical Inc. 16597 N. 92nd St Suite 101 Scotsdale, AZ 85260 USA



Legal Manufacturer
Biomet Sports Medicine
P.O. Box 587
56 E. Bell Drive
Warsaw, Indiana 46581-05

Warsaw, Indiana 46581-0587 USA

www.zimmerbiomet.com

