

A.L.P.S.[®] Proximal Humerus Plating System

Product Brochure



Two plating options for optimal subchondral support


The A.L.P.S. Proximal Humerus Plating System builds on the principle of Spatial Subchondral Support to deliver a flexible, efficient plating solution. The system creates a 3-dimensional scaffold to resist varus stress and was used successfully in its predecessors, the S^{3®} Proximal Humerus Plating System and the DVR[®] Anatomic Volar Plating System. This system offers the next generation in humeral plating by offering the surgeon two plating options based on fracture pattern and preference. It is designed to minimize the risk of complications commonly associated with the treatment of proximal humerus fractures:

- Minimizes varus collapse by creating an internal subchrondral support system of diverging and converging locking screws
- Minimizes articular surface screw penetration through the use of blunt-end pegs
- Minimizes subacromial impingement by using a low plate configuration that sits 2 cm distal to the greater tuberosity



Spatial Subchrondral Support helps minimize varus collapse.



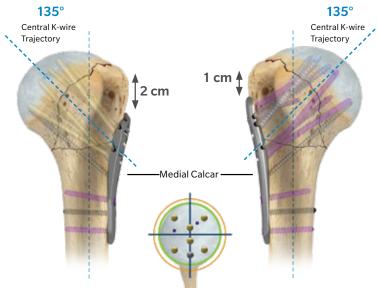

The **Low Plate** sits 2 cm from the greater tuberosity to allow for a greater range of motion.

The **High Plate** sits 1 cm from the greater tuberosity and offers two additional screw holes to achieve direct screw fixation of the greater tuberosity fragment.



Tapered, triple-lead locking and low-profile non-locking screw options provide optimal fixation. Cobalt chrome multi-directional locking screws allow for up to a 25° cone of angulation.



Pre-loaded, disposable F.A.S.T. Guide[®] Inserts aid in accurate drilling and offer reduced assembly, saving OR time.

A single **T15 driver** for all screws and pegs offers greater simplicity.



In-situ multi planar bending of the shaft provides customized contouring of the anatomic plates (11 and 14 hole plates only).

Designed to reduce the need to release the deltoid by using precontoured anterior curvature to navigate the deltopectoral interval.

References

 Compared to 316L electropolished stainless steel, color anodized titanium and machined titanium.

Laboratory results are not necessarily indicative of clinical performance.

INDICATIONS

The Biomet A.L.P.S. Proximal Humeral Plating System is indicated for fixation of fractures and fracture dislocations, fusions, osteotomies and non-unions of the humerus, particularly in osteopenic bone.

Patient selection factors to be considered include:

- 1. Need for alignment and stabilization of bone fractures
- Ability and willingness of the patient to follow postoperative care instructions until healing is complete
- 3. A good nutritional state of the patient.

This material is intended for healthcare professionals and the Zimmer Biomet sales force. Distribution to any other recipient is prohibited. For indications, contraindications, warnings, precautions, potential adverse effects and patient counseling information, see the package insert or contact your local representative; visit www.zimmerbiomet. com for additional product information. All content herein is protected by copyright, trademarks and other intellectual property rights, as applicable, owned by or licensed to Zimmer Biomet or its affiliates unless otherwise indicated, and must not be redistributed, duplicated or disclosed, in whole or in part, without the express written consent of Zimmer Biomet.

For indications, contraindications, warnings, precautions, potential adverse effects and patient counseling information, see the package insert or contact your local representative; visit www.zimmerbiomet. com for additional product information. Check for country product clearances and reference product specific instructions for use. Zimmer Biomet does not practice medicine. This technique was developed in conjunction with health care professional. This document is intended for surgeons and is not intended for laypersons. Each surgeon should exercise his or her own independent judgment in the diagnosis and treatment of an individual patient, and this information does not purport to replace the comprehensive training surgeons have received. As with all surgical procedures, the technique used in each case will depend on the surgeon's medical judgment as the best treatment for each patient. Results will vary based on health, weight, activity and other variables. Not all patients are candidates for this product and/or procedure. Caution: Federal (USA) law restricts this device to sale by or on the order of a surgeon. Rx only.

©2016, 2021 Zimmer Biomet



444

USA

Legal Manufacturer Biomet Trauma P.O. Box 587 56 East Bell Drive Warsaw, Indiana 46581-0587

www.zimmerbiomet.com

CONTRAINDICATIONS

- 1. Active infection.
- 2. Patient conditions including blood supply limitations, and insufficient quantity or quality of bone.
- Patients with mental or neurologic conditions who are unwilling or incapable of following postoperative care instructions or materials.
- 4. Foreign body sensitivity. Where material sensitivity is suspected, testing is to be completed prior to implantation of the device.

C€2797

CE mark on a surgical technique is not valid unless there is a CE mark on the product label.