






**Persona™ Fixed  
Resection Tower  
42-5099-006-00**

**Cleaning Instructions**

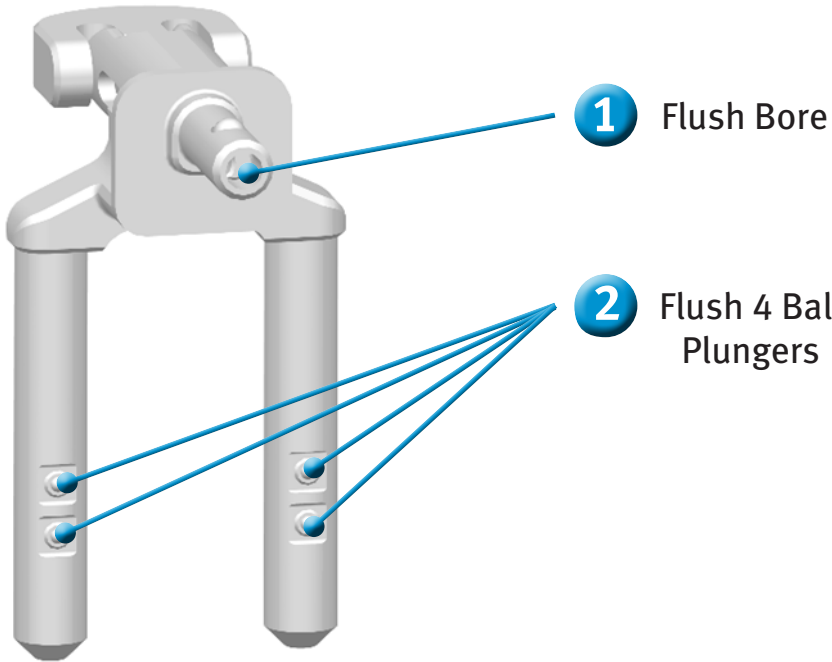

3 Flush Spring Cavity  
(top and bottom)

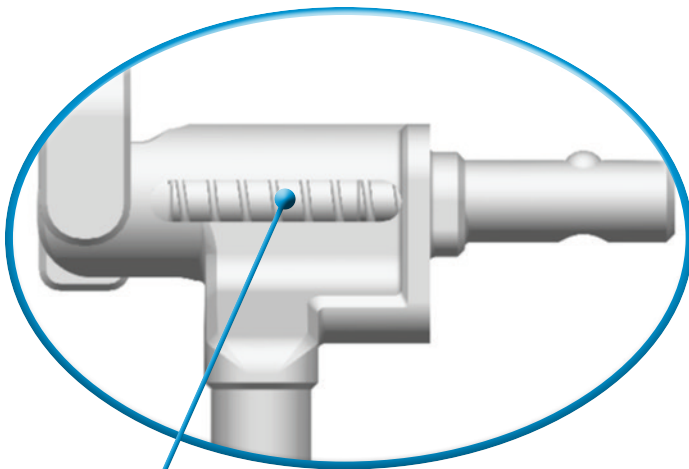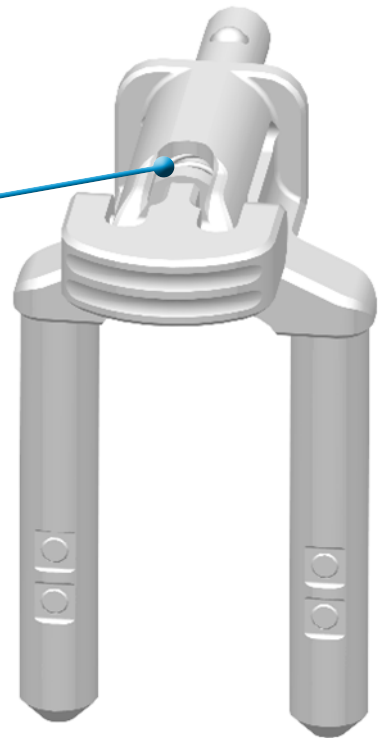

4 Flush Spring Cavity  
(both sides)